



Webly® Achilles TT™ Application

Warnings and Instructions: Review carefully, proper application is required


⚠ Warning: This device will not prevent or eliminate risk of injury. Do Not Overtighten. If swelling, pain, skin irritation, or an unusual reaction occurs, discontinue use immediately and consult your medical professional. For optimal performance wear over a sock.
Care: Hand wash using mild soap. Rinse thoroughly. Air dry only. Do not tumble dry.

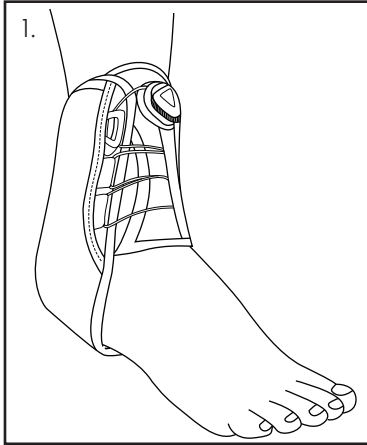


1. Slide foot into the gauntlet with laces loosely tightened.

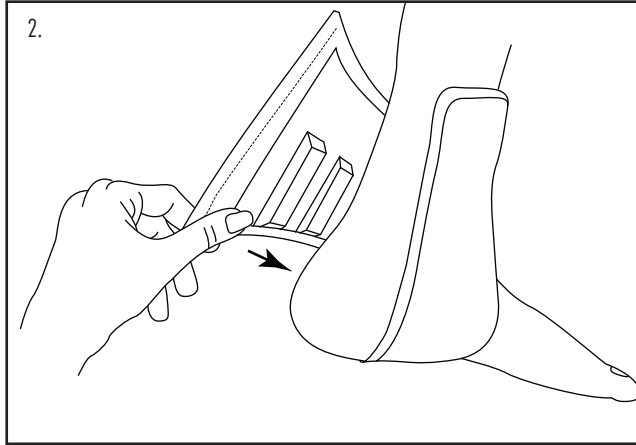


2. Apply posterior panel: Center the Achilles pads so the irritated tissues rest directly in between the two soft pads.

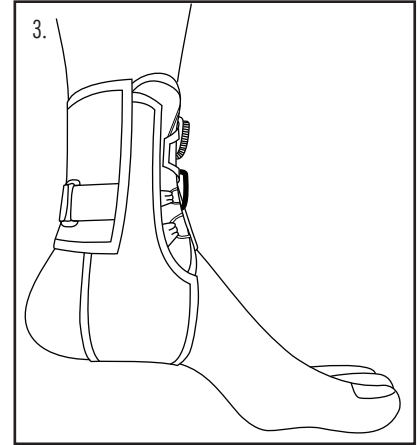


3. Secure hook and loop closures maintaining the pad position and repeat the process on the other side.

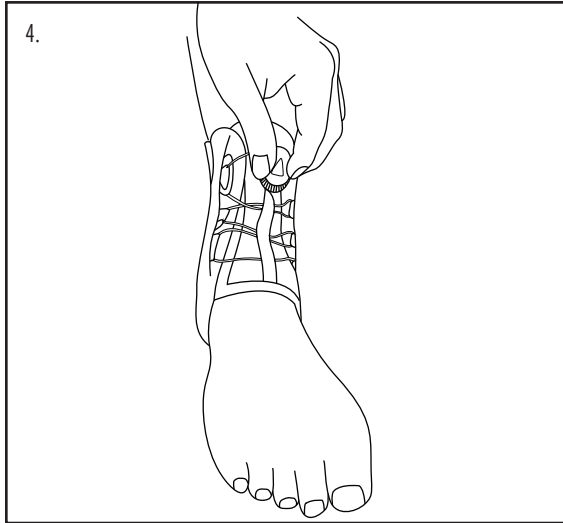


4. When back panel is secured, push in and turn the BOA® nob clockwise to tighten the lacing to create intimate fit of the gauntlet. Note: When tightened, pressure on both sides of the Achilles tendon should be felt.

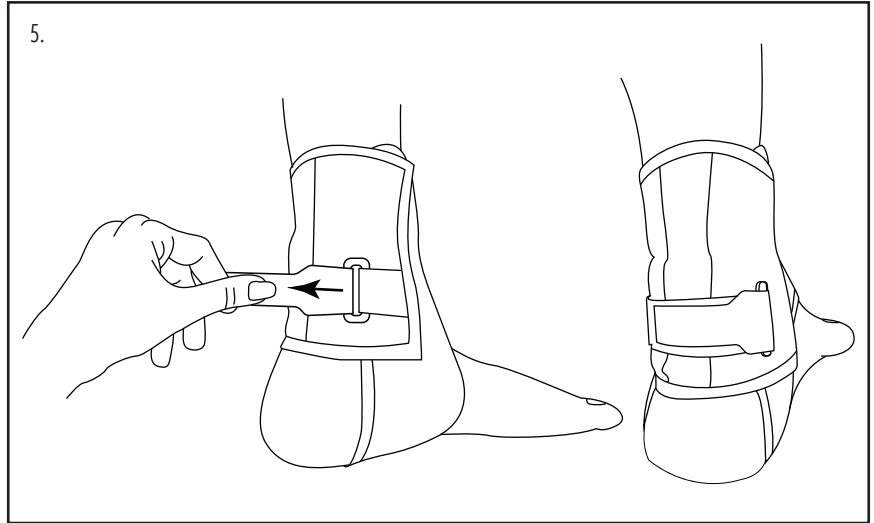

5. Pull the tendon tension adjustment tab to a comfortable tension so it compresses the tendon between to two pads (do not overtighten) application is now complete.

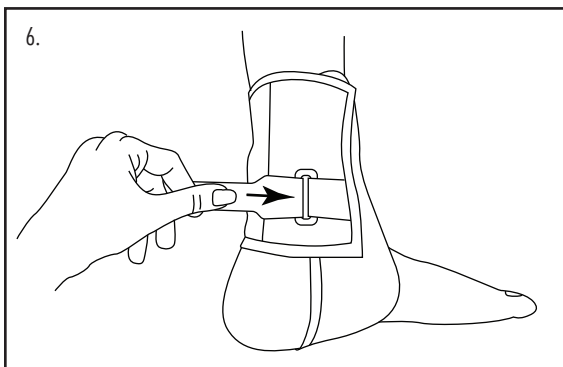

6. To remove the Webly® Achilles TT™: Loosen tendon strap, pull out on the BOA® nob, open the laces entirely.

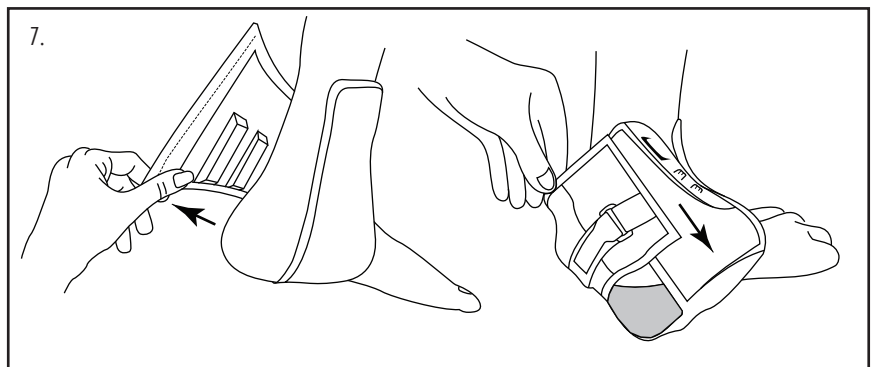

7. Undo lateral or medial side of the back panel and slide foot out OR slide brace over foot.

To Reapply: Slide foot in brace, make sure the two posterior pads approximate the tendon, tighten the BOA, cinch the tendon tension adjustment tab to a comfortable tension.



© 2023 Weber Orthopedics Inc.
DBA Hely & Weber all rights reserved

1185 E Main St., Santa Paula, California 93060
California: 800-221-5465, National: 800-654-3241
International: 805-525-4244, fax: 805-933-2348
U.S. fax: 800-559-5975, www.hely-weber.com

Rev A 08/24